


# Water Quality MultiMeasure Sensor

PS-2169

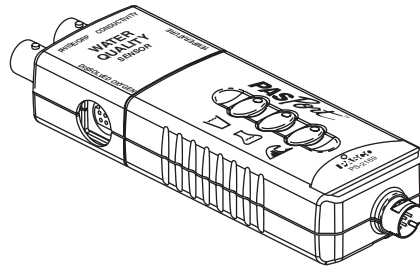

Included Equipment	Part Number
Water Quality MultiMeasure Sensor	PS-2169
Stainless Steel Temperature Probe	PS-2153
pH Electrode	699-195
Dissolved Oxygen (DO <sub>2</sub> ) Probe <sup>1</sup>	699-06320
Conductivity Electrode (10x)	699-06621
<b>Required Equipment</b>	
PASPORT Interface <sup>2</sup>	See PASCO catalog or <a href="http://www.pasco.com">www.pasco.com</a>
<b>Optional Equipment</b>	
Fast-response Temperature Probe	PS-2135 (3-pack)
Skin/surface Temperature Probe	PS-2131
Conductivity Electrode (1x)	699-06620
Various Ion-selective Electrodes (ISE)	See PASCO catalog or <a href="http://www.pasco.com">www.pasco.com</a>
Oxidation Reduction Potential (ORP) Electrode	CI-6716
DO <sub>2</sub> Electrode Maintenance Kit	CI-6541

<sup>1</sup> The DO<sub>2</sub> Probe comes with a bottle of filling solution, a syringe, a replacement membrane cartridge and O-ring, and a plunger. See illustration on page 7.

<sup>2</sup> PASPORT interfaces include the AirLink (IW-4100 or PS-2005), Xplorer GLX (PS-2002), Xplorer (PS-2000), PowerLink (PS-2001), and USB Link (PS-2100)

## Introduction

The PS-2169 Water Quality MultiMeasure Sensor combines four sensors in a single unit:

- Temperature
- Conductivity
- pH, ORP and ion-selective electrode voltage
- Dissolved Oxygen (DO<sub>2</sub>)

When connected to a PASPORT interface, the multi-sensor collects data at up to 20 samples per second from each component sensor. You can use just one component sensor at a time or any combination simultaneously. If you have a PASPORT interface that supports multiple sensors, or if you have more than one interface connected to your computer, you can use the Water Quality MultiMeasure Sensor in combination with other PASPORT sensors.

*Note: No electrical interference will occur between two or more probes connected to a single Water Quality MultiMeasure Sensor.*


## Sensor, Interface, and Software Setup

Connect the multi-sensor to your PASPORT interface as pictured (right). Connect any or all of the included probes to the multi-sensor. (You can leave any probe disconnected if you do not plan to use it.) If you will be using an ion-selective electrode or oxygen reduction potential electrode, connect it to the pH/ISE/ORP port.

Follow the instructions below to set up the multi-sensor with DataStudio software (if you are using a computer) or the Xplorer GLX (if you are using it standalone without a computer).

For detailed information about each of the multi-sensor's component sensors see "Temperature" on page 3, "Conductivity" on page 3, "pH/ISE/ORP" on page 4, and "Dissolved Oxygen" on page 6.

*Note: Only the tips and handles of the probes should be immersed in liquid, keep the cables, connectors and body of the multi-sensor dry.*

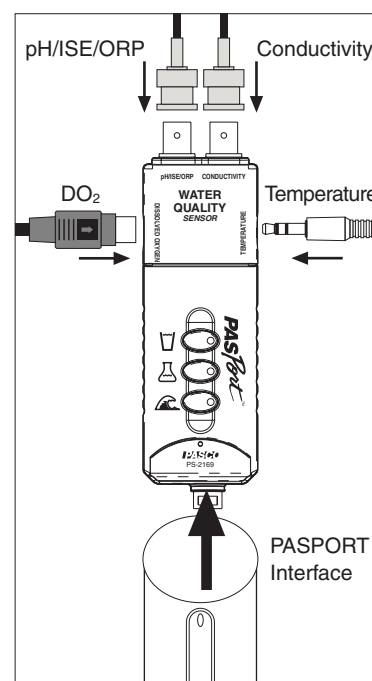


## DataStudio Setup


If you are using a computer, connect the PASPORT interface to the computer and start DataStudio. (Refer to the documentation that came with your PASPORT interface for instructions on connecting it to your computer.) In DataStudio, click the Start button to begin data collection; click the Stop button to stop data collection.

Note that the sensor may collect data for probes that are not connected. Hide or ignore these measurements. To hide measurements that you do not need, open the Experiment Setup Window by clicking the Setup button. In the Setup window you can also change the sampling rate and open the calibration dialog box (see Appendix A). For more instructions on using DataStudio, press F1 to open DataStudio's on-line help.



## Xplorer GLX Setup

If you are using an Xplorer GLX in standalone mode, press  to start data collection.

Note that the sensor may collect data for probes that are not connected. Hide or ignore these measurements. To hide measurements that you do not need, open the Sensors screen (from the Home screen, press ). In the Sensors screen you can also change the sampling rate and open the calibration dialog box. For more instructions on using the Xplorer GLX, refer to the GLX Users' Guide.

## Temperature

Use this component of the multi-sensor to measure the temperature of a fluid or object. The measurement can be displayed in units of °C, °F, or K. (In DataStudio, click the Setup button to change units.) You can use the included stainless steel probe or a different probe, such as the Fast-response Probe (PS-2135) or Skin/Surface Probe (PS-2131). PASCO physics apparatus containing an embedded 10 kΩ thermistor can also be connected to the multi-sensor. The multi-sensor automatically detects the presence of a temperature probe, and it will only collect temperature data if a probe is connected.

### Measuring Temperature

To measure temperature, connect the probe and start data collection. Immerse the tip of the probe in a fluid or place it in contact with an object. The included stainless steel probe can be used in both dry conditions and in liquids, such as water and other mild chemicals and solutions.

*Tip: For better chemical resistance, use a Teflon<sup>®</sup> cover (CI-6549).*

### Temperature Calibration

The temperature measurement can be calibrated; however, for most applications calibration is not necessary. Use a two-point calibration with two standards of known temperature. For instructions on calibrating in DataStudio, see Appendix A. For instructions on calibrating on the Xplorer GLX, refer to the Xplorer GLX Users' Guide.


## Conductivity

The conductivity component sensor measures the electrolytic conductivity of aqueous solutions. It determines the conductivity by applying an alternating voltage to the electrode cell at the end of the probe and measuring the resulting current. You can use the included 10x electrode or a 1x electrode (PASCO part 699-06620). In the software or on the interface select the **Conductivity (10x)** or **Conductivity (1x)** measurement, depending on which electrode you are using.

*Note: The 10x probe can be used to measure conductivity up to 100000 S/cm. The 1x probe has one tenth of the range (up to 10000 S/cm) but ten times better resolution.*

### Measuring Conductivity




Before using the conductivity electrode, soak the end in distilled water for 5 to 10 minutes. Connect the electrode to the multi-sensor and start data collection. Immerse

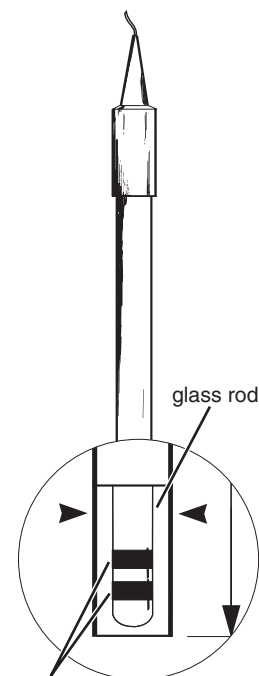

platinized  
platinum  
conductors

**Conductivity Electrode**

the end of the electrode in the solution to be measured and wait for the reading to stabilize. Rinse the electrode with deionized water before measuring a different solution.

The conductivity sensor has three ranges, which you select using the three buttons on the multi-sensor. To select a range, push one of the buttons:  for 0 S/cm to 1000 S/cm,  for 0 S/cm to 10000 S/cm, or  for 0 S/cm to 100000 S/cm. Lights on the buttons indicate which range is selected. To determine which range is appropriate, look at the data (on a Graph display, for instance) while it is being collected; if the measurement appears to be “railed” at the top of the selected range (1000 S/cm or 10000 S/cm), select the next higher range. You can push a button to change the range without stopping data collection.

*Note: The ranges specified above are for a 10x probe. Divide each range by 10 if you are using a 1x probe.*

The conductivity electrode is sensitive to very low concentrations of dissolved solids, so you will probably never measure a sample with a conductivity of zero. A reading of 25 S/cm for “pure” water is typical. True pure water is difficult to obtain and store. The table (right) lists typical conductivity values for common aqueous solutions at 25 °C.

As a rule of thumb, to estimate total dissolved solids (TDS) in parts per million (ppm), divide the conductivity in S/cm by 2:

$$\text{TDS (ppm)} = \frac{\text{Conductivity ( S/cm)}}{2}$$

## Conductivity Calibration

The conductivity measurement can be calibrated; however, for most applications calibration is not necessary. Use a one-point calibration with a standard solution of known conductivity. For instructions on preparing a standard solution, see Appendix C. For instructions on calibrating in DataStudio, see Appendix A. For instructions on calibrating on the Xplorer GLX, refer to the Xplorer GLX Users’ Guide.

## Conductivity Electrode Maintenance And Storage

To ensure accurate and reproducible results, the electrode must be clean. Substances on the electrode may contaminate the solution being tested and change the conductivity. To clean the electrode, dip the end into a detergent solution or dilute nitric acid (1%) and stir for three minutes, then rinse with deionized water.


For storage, dry the electrode and return it to its box. Before use, soak the electrode in distilled water for at least 5 minutes.

## pH/ISE/ORP

The pH/ISE/ORP input of the multi-sensor is a specialized voltage sensor. Its BNC connector accepts the included pH electrode, as well as ISE and ORP electrodes. The sensor measures the voltage produced by any of these electrodes. When used with a pH probe, the sensor also computes the pH based on the measured voltage.

Connect the pH electrode (or other electrode) to the pH/ISE/ORP port and start data collection. On your computer or interface, display the **ISE Voltage** measurement (this measurement is valid for pH and ORP electrodes as well as ISE) or the **pH** measurement for the calculated pH (assuming that the pH electrode is connected).

**Range** (μS/cm) 10x probe



Solution	Conductivity ( S/cm)
Ultra-pure Water	0.05 to 0.75
Drinking Water	50 to 1500
Ocean Water	~53000

## Measuring pH

The pH electrode produces a voltage proportional to the pH of the solution that it is immersed in. This voltage is measured by the multi-sensor, which computes pH.

Unscrew and remove the storage bottle from the electrode (be careful not to spill the storage solution). Push the O-ring and bottle cap up the electrode handle. Rinse the electrode tip with distilled water. If you see bubbles in the electrode bulb, gently shake the electrode downward (similar to shaking down a thermometer). Start data collection. Place the tip of the electrode in the solution to be measured and wait for the reading on your computer or interface to stabilize. Rinse the electrode with distilled water before measuring another solution.

## pH Calibration

The pH measurement can be calibrated; however, for most applications calibration is not necessary. Perform a two-point calibration with two buffer solutions of known pH. For instructions on calibrating in DataStudio, see Appendix A. For instructions on calibrating on the Xplorer GLX, refer to the Xplorer GLX Users' Guide.

## pH Electrode Maintenance and Storage

### Cleaning

If the pH electrode becomes contaminated, use one of these methods to clean and restore it. After any of these procedures, soak the electrode in a pH 7 buffer solution for 30 minutes.

- **General Contamination:** Soak the electrode in 0.1 molar hydrochloric acid (HCl) for 15 minutes.
- **Protein Deposits:** Soak the electrode in a solution of 1% pepsin in 0.1 molar HCl.
- **Inorganic Deposits:** Rinse the electrode with 0.1 molar ethylene dinitric tetra-acidic acid (EDTA) tetrasodium solution.
- **Oil and Grease Film:** Wash the electrode carefully in a mild detergent or a solvent known to be effective for the particular film.
- **Unknown Contamination:** Soak the electrode alternately in 12 molar sodium hydroxide (NaOH) and 1 molar HCl. Leave it in each solution for one minute. Rinse completely between soakings. End with HCl. (The NaOH etches the glass and the HCl reestablishes hydrogen ions on the surface.)

If these steps fail to improve the response of the electrode, replaced it.

### Storage

Store the pH electrode in the included electrode storage bottle with one of the following solutions. (Never store the electrode in distilled water.)


- **Short-term** (up to one week): pH 4 buffer solution or tap water.
- **Long-term** (over one week): pH 4 buffer solution with 1 g per 100 mL of potassium chloride (KCl) added.

## Dissolved Oxygen

The DO<sub>2</sub> component of the multi-sensor is designed for use in aqueous media at temperatures ranging from 0 °C to 50 °C. For greatest accuracy, the following requirements should be met:

- Although the unit is temperature compensated, it should be calibrated at approximately the same temperature as the test solution.
- The sensor must equilibrate for a short period when the temperature of the test solution changes.
- The test solution should constantly flow past the membrane of the probe. This can be accomplished by gently swirling the electrode during measurement.

The DO<sub>2</sub> probe consists of a platinum (Pt) cathode and a silver (Ag) anode surrounded by potassium chloride (KCl<sub>(aq)</sub>) electrolyte filling solution with a silicon membrane separating the filling solution from the test solution. When the probe is placed in an aqueous medium that contains dissolved oxygen, O<sub>2</sub> molecules diffuse across the membrane and react with water molecules (H<sub>2</sub>O) in the presence of electrons from the cathode to form hydroxide ions (OH<sup>-</sup>). Hydroxide ions diffuse to the anode and react with silver atoms, forming silver oxide (Ag<sub>2</sub>O), H<sub>2</sub>O, and free electrons. The net movement of negative charge (electrons) from the cathode to the anode is measured by the sensor as an electric current. Since the rate of O<sub>2</sub> diffusion across the membrane is proportional DO<sub>2</sub> concentration, the rate of these reactions and the resulting electric current is also proportional to DO<sub>2</sub> concentration. The rate at which the probe processes oxygen also depends on temperature. To correct for temperature variation, the probe contains a temperature-sensing thermistor, which adjusts the gain of an amplifier in the multi-sensor.

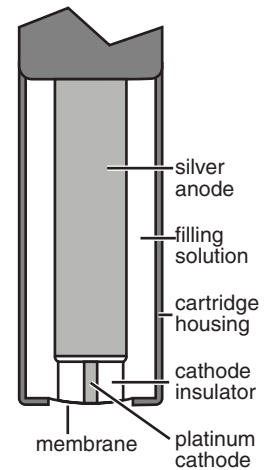


Detail of DO<sub>2</sub> Probe Tip

### Adding Filling Solution

Prior to its initial use, and after long-term storage or cleaning, prepare the probe by filling it with electrolyte solution as follows:


1. Remove the storage bottle from the end of the probe.
2. Unscrew and remove the cartridge housing at the end of the probe, as illustrated (right).
3. Pull about 10 mL of new filling solution into the syringe (included with the probe). Be careful not to introduce air bubbles.
4. Place the tip of the syringe in the cartridge housing, very close to—but not touching—the membrane. Slowly fill the housing to about 5 mm from the top. Agitate the housing while filling to avoid introducing air bubbles.
5. Replace the housing over the electrode and screw it into place. Excess filling solution will spill from the housing as you do this.
6. Rinse and dry the outside of the probe.

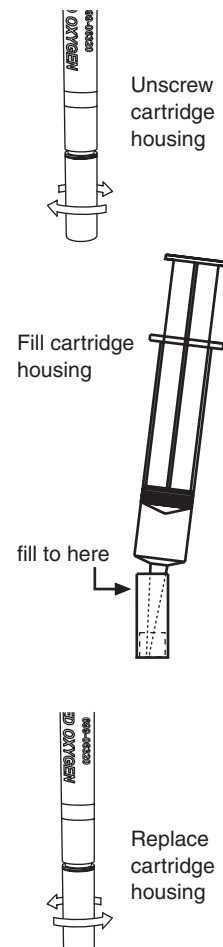

## DO<sub>2</sub> Calibration

Perform a one-point calibration using 100% humidified air as the known standard, which is equivalent to 100% saturated (pure) water. Prepare 100% humidified air as follows:

1. Place about 5 mL (to a height of about 1 cm) of deionized water into a clean electrode storage bottle.
2. Slip the cap and O-ring of the soaker bottle over the end of the probe. Insert the probe into the soaker bottle and screw on the cap. Adjust the height of the end of the probe to about 2 cm above the water.
3. Shake the probe and bottle vigorously for about 10 seconds. Shake off any large water drops from the membrane.
4. Hold the probe vertically so that it is in the air *above* the water, not in the water itself.
5. Perform a one-point calibration on either the **Dissolved Oxygen (%)** or **Dissolved Oxygen (mg/L)** measurement. If you are calibrating the percentage measurement, enter "100" as the known value. If you are calibrating the mg/L measurement, look up the known concentration in Appendix D. For instructions on calibrating in DataStudio, see Appendix A. For instructions on calibrating on the Xplorer GLX, refer to the Xplorer GLX Users' Guide.

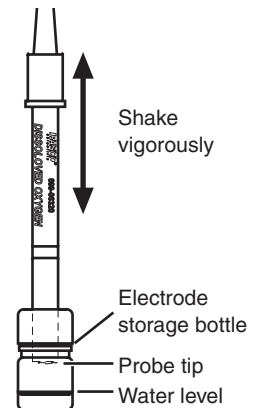


Preparation of 100% humidified air for calibration

## Measuring DO<sub>2</sub>

Follow the instructions above to fill the probe with electrolyte solution and calibrate the measurement. Start data collection. Remove the storage bottle from the probe. Immerse the end of the probe in the solution to be measured. Gently swirl the probe or stir the solution to prevent localized oxygen depletion at the probe end. Wait for the reading to stabilize. Rinse the electrode with deionized water before measuring a different solution.

## DO<sub>2</sub> Probe Maintenance and Storage


The probe comes with extra filling solution, a replacement membrane cartridge and O-ring, and a plunger for installing the cartridge. Order the Electrode Maintenance Kit (CI-6541) to replace these items.

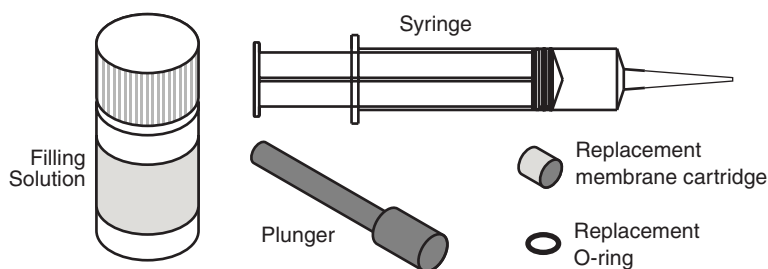

### Electrode Cleaning

To maintain optimal performance, periodically clean the silver electrode and replace the electrolyte filling solution as follows:

1. Unscrew and remove the cartridge housing at the end of the probe. Discard the old filling solution from the cartridge housing.

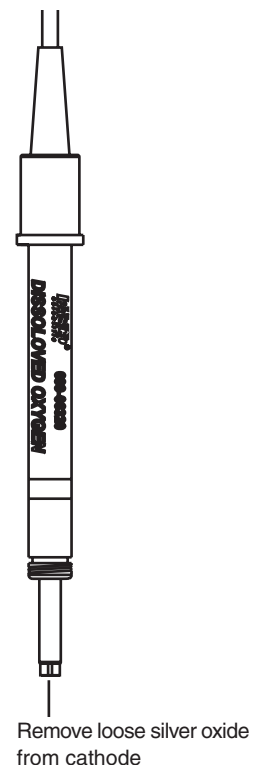

2. Rinse the electrode with tap water (or deionized water in areas with hard tap water) and rub it with a paper towel to dry it and remove loose silver oxide.
3. Follow the “Adding Filling Solution” instructions on page 6 to fill and reassemble the probe.



### Membrane Replacement

If the silicon membrane is damaged or not performing optimally, replace the membrane cartridge as follows:

1. Unscrew and remove the cartridge housing at the end of the probe. Discard the old filling solution from the cartridge housing.
2. Use the plunger to push the membrane cartridge into and through the housing so that it comes out through the threaded end of the housing, as illustrated (right).
3. Examine the O-ring in the housing. If it is damaged, remove it with fine-tipped tweezers and insert the replacement.
4. Use the plunger to push the replacement cartridge into the housing until it is seated at the tip of the housing.
5. Follow the “Adding Filling Solution” instructions on page 6 to fill and reassemble the probe.

### Storage

- **Short-term** (up to two weeks): Add about 10 ml of deionized water to the electrode storage bottle and place it over the end of the probe. Store the probe and bottle in a sealed plastic bag.
- **Long-term** (over two weeks): Follow the “Electrode Cleaning” instructions below, but do not refill the probe. Rinse the cartridge housing and storage bottle with tap water. Allow all parts to dry before reassembling them.

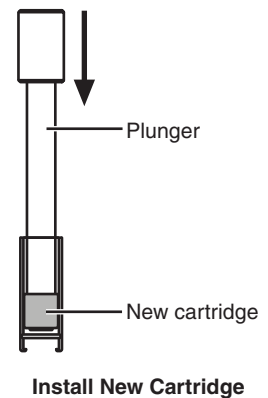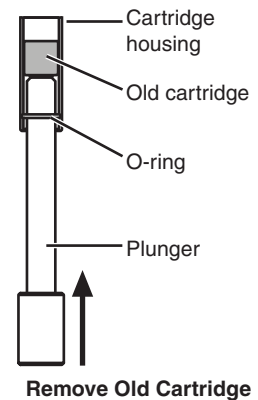



## Specifications

<b>General</b>	
<b>Component Sensors</b>	Temperature, Conductivity, pH/ISE/ORP probe voltage, Dissolved Oxygen
<b>Max. Sampling Rate</b>	20 samples per second (for each component sensor)
<b>Default Sampling Rate</b>	2 samples per second
<b>Temperature</b>	
<b>Range</b>	-35 °C to +135 °C
<b>Accuracy</b>	±0.5 °C
<b>Resolution</b>	0.01 °C or better
<b>Sensing Element</b>	10 kΩ thermistor located in probe tip
<b>Conductivity</b>	
<b>Range</b>	three user-selectable ranges: 0 to 1000 S/cm, 0 to 10000 S/cm, 0 to 100000 S/cm with included 10x probe 0 to 100 S/cm, 0 to 1000 S/cm, 0 to 10000 S/cm with optional 1x probe
<b>Accuracy</b>	±10% of full scale without calibration
<b>Resolution</b>	better than 0.05% of full scale
<b>pH/ISE/ORP probe voltage</b>	
<b>Electrode Connector</b>	standard BNC
<b>Input Resistance</b>	1012 Ω
<b>Voltage Range</b>	-2000 mV to +2000 mV
<b>Voltage Resolution</b>	0.1 mV
<b>pH Range</b>	0 to 14
<b>pH Resolution</b>	0.001
<b>Dissolved Oxygen</b>	
<b>Range</b>	0 to 20 mg/L
<b>Accuracy</b>	±0.2 mg/L after calibration ±2 mg/L without calibration
<b>Resolution</b>	0.01 mg/L
<b>Temperature Range</b>	0 °C to 50 °C

## Appendix A: DataStudio Calibration

In DataStudio, click the Setup button to open the Experiment Setup window; in that window, click the Calibrate button to open the Calibrate Sensors dialog box. Use a two-point calibration for temperature or pH. Use a one-point calibration (next page) for conductivity or dissolved oxygen.

### Two-point Calibration

For a two-point calibration, you will need two “known standards,” such as two buffer solutions of known pH or two liquids of known temperature.


1. From the Sensor field, select **Water Quality**.
2. From the Measurement field, select **Temperature or pH**.
3. Ensure that “Calibrate all similar measurements simultaneously” is *not* selected.
4. From the Calibration Type menu, select **2 Point (Adjust Slope and Offset)**, if it is not already selected.
5. Place the temperature or pH probe in the first known standard.
6. Enter the known temperature or pH of the standard in the **Standard Value** field for Point 1.
7. Observe the **Present Sensor Measurement** and wait until it has stabilized.
8. Click the **Read From Sensor** button for Point 1.
9. Place the probe in the second known standard.
10. Enter the known temperature or pH of the standard in the **Standard Value** field for Point 2.
11. Observe the **Present Sensor Measurement** and wait until it has stabilized.
12. Click the **Read From Sensor** button for Point 2.
13. Click **OK** to accept the new calibration.

The screenshot shows the 'Calibrate Sensors' dialog box in DataStudio. The 'Sensor' dropdown is set to 'Water Quality' and the 'Measurement' dropdown is set to 'Temperature (°C)'. The checkbox 'Calibrate all similar measurements simultaneously' is unchecked. Under 'Previous Calibration', the slope is 1.000 Units/°C and the offset is 0.000 Units. The 'Present Sensor Measurement' shows 24.80 °C and 24.80 Units. The 'Calibration Type' is set to '2 Point (Adjust Slope and Offset)'. There are two calibration points: Point 1 with a Standard Value of 0.000 °C and a Sensor Value of 0.000 Units; Point 2 with a Standard Value of 100.0 °C and a Sensor Value of 100.0 Units. The 'New Calibration' section shows a slope of 1.000 Units/°C and an offset of 0.000 Units. Buttons for 'Read From Sensor', 'OK', and 'Cancel' are at the bottom.

## One-point Calibration


A one-point slope calibration requires one known standard. For conductivity, use one of the solutions in Appendix C. For dissolved oxygen, use 100% humidified air (see “DO<sub>2</sub> Calibration” on page 7 for details).

1. From the Sensor field, select **Water Quality**.
2. From the Measurement field, select **Dissolved Oxygen (mg/L), Dissolved Oxygen (%), Conductivity (1X Probe), or Conductivity (10X Probe)**.
3. Ensure that “Calibrate all similar measurements simultaneously” is *not* selected.
4. From the Calibration Type menu, select **1 Point (Adjust Slope Only)**, if it is not already selected.
5. Place the probe in the known standard.
6. Enter the known conductivity or DO<sub>2</sub> concentration in the **Standard Value field** for Point 2.
7. Observe the **Present Sensor Measurement** and wait until it has stabilized. (For conductivity, ensure that the present measurement is within the selected sensor range. If it is not, press a button on the multi-sensor to select a higher range.)
8. Click the **Read From Sensor** button for Point 2.
9. Click **OK** to accept the new calibration.

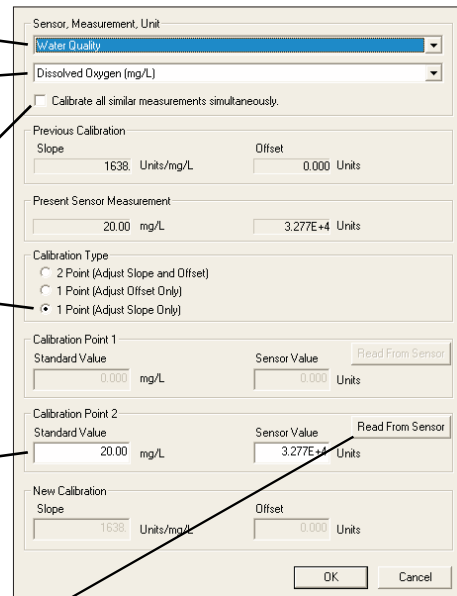

## Appendix B: EZ Screen

If you are using the Water Quality MultiMeasure Sensor with a PASPORT interface connected to a computer, you can use EZ-Screen software instead of DataStudio. When the sensor is connected to the computer through the interface (if DataStudio is not running) a window automatically launches giving you the option of launching EZ-Screen. In EZ-Screen, click the green arrow button to start data collection. Click the Water Quality icon in the lower-right corner to cycle through temperature, dissolved oxygen, probe voltage, conductivity, and pH measurements.



**EZ-Screen**

## Appendix C: Reference Solutions for Conductivity Calibration

Reference Solution	Approximation Normality of Solution	Method of Preparation	Temperature (°C)	Electrical Conductivity <sup>1</sup> (µS/cm)
A	1	74.2480 g of KCl weighed in air per 1 L of solution at 20 °C	0	65176
			18	97838
			25	111342
B	0.1	7.4365 g of KCl weighed in air per 1 L of solution at 20 °C	0	7138
			18	11167
			25	12856
C	0.01	0.7440 g of KCl weighed in air per 1 L of solution at 20 °C	0	773.6
			18	1220.5
			25	1408.6
D	0.001	Dilute 100 mL of solution C to 1 L at 20 °C	0	77.69
			18	127.54
			25	148.93

<sup>1</sup>Excluding the conductivity of the water used to prepare the solutions. These tabulated conductivity values are in international units. When using measuring instruments calibrated in absolute units, multiply the tabular values by 0.999505

## Appendix D: DO<sub>2</sub> Calibration Tables

**Table 1: DO<sub>2</sub> Versus Temperature and Pressure**

Note: Atmospheric pressures from 695 to 600 mm Hg begin on page 14.

This table lists the absolute DO<sub>2</sub> concentration of 100% saturated pure water at various temperature and pressures. Multiply the pure-water figure by the correction factor from Table 2 (page 16) to determine the absolute concentration of a 100% saturated saline water sample.

Temp. °C	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
	795 (31.30)	790 (31.10)	785 (30.91)	780 (30.71)	775 (30.51)	770 (30.31)	765 (30.12)	760 (29.92)	755 (29.72)	750 (29.53)	745 (29.33)	740 (29.13)	735 (28.94)	730 (28.74)	725 (28.54)	720 (28.35)	715 (28.15)	710 (27.95)	705 (27.76)	700 (27.56)
0.0	15.3	15.2	15.1	15.0	14.9	14.8	14.7	14.6	14.5	14.4	14.3	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4
0.5	15.1	15.0	14.9	14.8	14.7	14.6	14.5	14.4	14.3	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.2
1.0	14.8	14.7	14.7	14.6	14.5	14.4	14.3	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.2	13.2	13.1
1.5	14.6	14.5	14.5	14.4	14.3	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.2	13.2	13.1	13.0	12.9
2.0	14.4	14.3	14.3	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7
2.5	14.2	14.2	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.6	12.5
3.0	14.1	14.0	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.6	12.5	12.5	12.4
3.5	13.9	13.8	13.7	13.6	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.6	12.6	12.5	12.4	12.3	12.2
4.0	13.7	13.6	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.6	12.6	12.5	12.4	12.3	12.2	12.1	12.0
4.5	13.5	13.4	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.7	12.6	12.5	12.4	12.3	12.2	12.1	12.1	12.0	11.9

Temp. °C	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
	795 (31.30)	790 (31.10)	785 (30.91)	780 (30.71)	775 (30.51)	770 (30.31)	765 (30.12)	760 (29.92)	755 (29.72)	750 (29.53)	745 (29.33)	740 (29.13)	735 (28.94)	730 (28.74)	725 (28.54)	720 (28.35)	715 (28.15)	710 (27.95)	705 (27.76)	700 (27.56)
5.0	13.3	13.3	13.2	13.1	13.0	12.9	12.8	12.7	12.7	12.6	12.5	12.4	12.3	12.2	12.2	12.1	12.0	11.9	11.8	11.7
5.5	13.2	13.1	13.0	12.9	12.8	12.7	12.7	12.6	12.5	12.4	12.3	12.2	12.2	12.1	12.0	11.9	11.8	11.7	11.7	11.6
6.0	13.0	12.9	12.8	12.8	12.7	12.6	12.5	12.4	12.3	12.3	12.2	12.1	12.0	11.9	11.8	11.8	11.7	11.6	11.5	11.4
6.5	12.8	12.8	12.7	12.6	12.5	12.4	12.3	12.3	12.2	12.1	12.0	11.9	11.9	11.8	11.7	11.6	11.5	11.5	11.4	11.3
7.0	12.7	12.6	12.5	12.4	12.4	12.3	12.2	12.1	12.0	12.0	11.9	11.8	11.7	11.6	11.6	11.5	11.4	11.3	11.2	11.1

7.5	12.5	12.4	12.4	12.3	12.2	12.1	12.0	12.0	11.9	11.8	11.7	11.6	11.6	11.5	11.4	11.3	11.3	11.2	11.1	11.0
8.0	12.4	12.3	12.2	12.1	12.1	12.0	11.9	11.8	11.7	11.7	11.6	11.5	11.4	11.3	11.3	11.2	11.1	11.0	11.0	10.9
8.5	12.2	12.1	12.1	12.0	11.9	11.8	11.8	11.7	11.6	11.5	11.4	11.4	11.3	11.2	11.1	11.1	11.0	10.9	10.8	10.7
9.0	12.1	12.0	11.9	11.8	11.8	11.7	11.6	11.5	11.5	11.4	11.3	11.2	11.2	11.1	11.0	10.9	10.8	10.8	10.7	10.6
9.5	11.9	11.9	11.8	11.7	11.6	11.6	11.5	11.4	11.3	11.2	11.2	11.1	11.0	10.9	10.9	10.8	10.7	10.6	10.6	10.5

10.0	11.8	11.7	11.6	11.6	11.5	11.4	11.3	11.3	11.2	11.1	11.0	11.0	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.4
10.5	11.7	11.6	11.5	11.4	11.4	11.3	11.2	11.1	11.1	11.0	10.9	10.8	10.8	10.7	10.6	10.5	10.5	10.4	10.3	10.2
11.0	11.5	11.4	11.4	11.3	11.2	11.2	11.1	11.0	10.9	10.9	10.8	10.7	10.6	10.6	10.5	10.4	10.3	10.3	10.2	10.1
11.5	11.4	11.3	11.2	11.2	11.1	11.0	11.0	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.4	10.3	10.2	10.2	10.1	10.0
12.0	11.3	11.2	11.1	11.0	11.0	10.9	10.8	10.8	10.7	10.6	10.5	10.5	10.4	10.3	10.3	10.2	10.1	10.0	10.0	9.9
12.5	11.1	11.1	11.0	10.9	10.8	10.8	10.7	10.6	10.6	10.5	10.4	10.4	10.3	10.2	10.1	10.1	10.0	9.9	9.9	9.8
13.0	11.0	10.9	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.4	10.3	10.2	10.2	10.1	10.0	10.0	9.9	9.8	9.7	9.7
13.5	10.9	10.8	10.7	10.7	10.6	10.5	10.5	10.4	10.3	10.3	10.2	10.1	10.1	10.0	9.9	9.8	9.8	9.7	9.6	9.6

14.0	10.8	10.7	10.6	10.6	10.5	10.4	10.4	10.3	10.2	10.1	10.1	10.0	9.9	9.9	9.8	9.7	9.7	9.6	9.5	9.5
14.5	10.6	10.6	10.5	10.4	10.4	10.3	10.2	10.2	10.1	10.0	10.0	9.9	9.8	9.8	9.7	9.6	9.6	9.5	9.4	9.4
15.0	10.5	10.5	10.4	10.3	10.3	10.2	10.1	10.1	10.0	9.9	9.9	9.8	9.7	9.7	9.6	9.5	9.5	9.4	9.3	9.3
15.5	10.4	10.4	10.3	10.2	10.2	10.1	10.0	10.0	9.9	9.8	9.8	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.2	9.2
16.0	10.3	10.2	10.2	10.1	10.0	10.0	9.9	9.8	9.8	9.7	9.7	9.6	9.5	9.5	9.4	9.3	9.3	9.2	9.1	9.1

16.5	10.2	10.1	10.1	10.0	9.9	9.9	9.8	9.7	9.7	9.6	9.5	9.5	9.4	9.4	9.3	9.2	9.2	9.1	9.0	9.0
17.0	10.1	10.0	10.0	9.9	9.8	9.8	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.3	9.2	9.1	9.1	9.0	8.9	8.9
17.5	10.0	9.9	9.9	9.8	9.7	9.7	9.6	9.5	9.5	9.4	9.3	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.8	8.8
18.0	9.9	9.8	9.8	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.3	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.7	8.7
18.5	9.8	9.7	9.7	9.6	9.5	9.5	9.4	9.3	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.8	8.8	8.7	8.7	8.6

19.0	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.3	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.8	8.7	8.6	8.6	8.5
19.5	9.6	9.5	9.5	9.4	9.3	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.5	8.5	8.4
20.0	9.5	9.4	9.4	9.3	9.3	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.5	8.4	8.3
20.5	9.4	9.3	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.3
21.0	9.3	9.2	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.5	8.4	8.4	8.3	8.2	8.2

21.5	9.2	9.2	9.1	9.0	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.3	8.2	8.1	8.1
22.0	9.1	9.1	9.0	9.0	8.9	8.8	8.8	8.7	8.7	8.6	8.5	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.1	8.0
22.5	9.0	9.0	8.9	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9
23.0	9.0	8.9	8.8	8.8	8.7	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.3	8.2	8.1	8.1	8.0	8.0	7.9	7.9
23.5	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.1	8.0	8.0	7.9	7.8	7.8

24.0	8.8	8.7	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7
24.5	8.7	8.7	8.6	8.5	8.5	8.4	8.4	8.3	8.3	8.2	8.1	8.1	8.0	8.0	7.9	7.9	7.8	7.7	7.7	7.6
25.0	8.6	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.2	8.1	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.7	7.6	7.6
25.5	8.5	8.5	8.4	8.4	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5
26.0	8.5	8.4	8.4	8.3	8.3	8.2	8.1	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.5	7.4
26.5	8.4	8.3	8.3	8.2	8.2	8.1	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4

Temp.	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
°C	795 (31.30)	790 (31.10)	785 (30.91)	780 (30.71)	775 (30.51)	770 (30.31)	765 (30.12)	760 (29.92)	755 (29.72)	750 (29.53)	745 (29.33)	740 (29.13)	735 (28.94)	730 (28.74)	725 (28.54)	720 (28.35)	715 (28.15)	710 (27.95)	705 (27.76)	700 (27.56)
27.0	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3
27.5	8.2	8.2	8.1	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.7	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2
28.0	8.2	8.1	8.1	8.0	8.0	7.9	7.9	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2

28.5	8.1	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.1	7.1
29.0	8.0	8.0	7.9	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0
29.5	8.0	7.9	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0
30.0	7.9	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9
30.5	7.8	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9

31.0	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8
31.5	7.7	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7
32.0	7.6	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7
32.5	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6
33.0	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6

33.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5
34.0	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.5
34.5	7.3	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.5	6.4
35.0	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3
35.5	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3

36.0	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2
36.5	7.1	7.0	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2
37.0	7.0	7.0	6.9	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1
37.5	7.0	6.9	6.9	6.8	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1
38.0	6.9	6.9	6.8	6.8	6.7	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0

38.5	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0
39.0	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	6.0
39.5	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	6.0	5.9
40.0	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.9

Temp.	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
°C	695 (27.36)	690 (27.17)	685 (26.97)	680 (26.77)	675 (26.57)	670 (26.38)	665 (26.18)	660 (25.98)	655 (25.79)	650 (25.59)	645 (25.39)	640 (25.20)	635 (25.00)	630 (24.80)	625 (24.61)	620 (24.41)	615 (24.21)	610 (24.02)	605 (23.82)	600 (23.62)
0.0	13.3	13.2	13.1	13.0	12.9	12.8	12.8	12.7	12.6	12.5	12.4	12.3	12.2	12.1	12.0	11.9	11.8	11.7	11.6	11.5
0.5	13.1	13.1	13.0	12.9	12.8	12.7	12.6	12.5	12.4	12.3	12.2	12.1	12.0	11.9	11.8	11.7	11.6	11.5	11.4	11.3
1.0	13.0	12.9	12.8	12.7	12.6	12.5	12.4	12.3	12.2	12.1	12.0	11.9	11.8	11.7	11.6	11.6	11.5	11.4	11.3	11.2
1.5	12.8	12.7	12.6	12.5	12.4	12.3	12.2	12.1	12.0	12.0	11.9	11.8	11.7	11.6	11.5	11.4	11.3	11.2	11.1	11.0
2.0	12.6	12.5	12.4	12.3	12.2	12.2	12.1	12.0	11.9	11.8	11.7	11.6	11.5	11.4	11.3	11.2	11.1	11.1	11.0	10.9

2.5	12.4	12.4	12.3	12.2	12.1	12.0	11.9	11.8	11.7	11.6	11.5	11.4	11.4	11.3	11.2	11.1	11.0	10.9	10.8	10.7
3.0	12.3	12.2	12.1	12.0	11.9	11.8	11.7	11.7	11.6	11.5	11.4	11.3	11.2	11.1	11.0	10.9	10.9	10.8	10.7	10.6
3.5	12.1	12.0	11.9	11.8	11.8	11.7	11.6	11.5	11.4	11.3	11.2	11.1	11.1	11.0	10.9	10.8	10.7	10.6	10.5	10.4
4.0	12.0	11.9	11.8	11.7	11.6	11.5	11.4	11.3	11.3	11.2	11.1	11.0	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.3
4.5	11.8	11.7	11.6	11.5	11.5	11.4	11.3	11.2	11.1	11.0	10.9	10.9	10.8	10.7	10.6	10.5	10.4	10.3	10.3	10.2

5.0	11.6	11.6	11.5	11.4	11.3	11.2	11.1	11.1	11.0	10.9	10.8	10.7	10.6	10.5	10.5	10.4	10.3	10.2	10.1	10.0
-----	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------	------

Temp. °C	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
	695 (27.36)	690 (27.17)	685 (26.97)	680 (26.77)	675 (26.57)	670 (26.38)	665 (26.18)	660 (25.98)	655 (25.79)	650 (25.59)	645 (25.39)	640 (25.20)	635 (25.00)	630 (24.80)	625 (24.61)	620 (24.41)	615 (24.21)	610 (24.02)	605 (23.82)	600 (23.62)
5.5	11.5	11.4	11.3	11.2	11.2	11.1	11.0	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.3	10.2	10.2	10.1	10.0	9.9
6.0	11.4	11.3	11.2	11.1	11.0	10.9	10.9	10.8	10.7	10.6	10.5	10.4	10.4	10.3	10.2	10.1	10.0	9.9	9.9	9.8
6.5	11.2	11.1	11.0	11.0	10.9	10.8	10.7	10.6	10.6	10.5	10.4	10.3	10.2	10.1	10.1	10.0	9.9	9.8	9.7	9.7
7.0	11.1	11.0	10.9	10.8	10.7	10.7	10.6	10.5	10.4	10.3	10.3	10.2	10.1	10.0	9.9	9.9	9.8	9.7	9.6	9.5

7.5	10.9	10.9	10.8	10.7	10.6	10.5	10.5	10.4	10.3	10.2	10.1	10.1	10.0	9.9	9.8	9.7	9.7	9.6	9.5	9.4
8.0	10.8	10.7	10.6	10.6	10.5	10.4	10.3	10.2	10.2	10.1	10.0	9.9	9.9	9.8	9.7	9.6	9.5	9.5	9.4	9.3
8.5	10.7	10.6	10.5	10.4	10.4	10.3	10.2	10.1	10.0	10.0	9.9	9.8	9.7	9.7	9.6	9.5	9.4	9.3	9.3	9.2
9.0	10.5	10.5	10.4	10.3	10.2	10.2	10.1	10.0	9.9	9.8	9.8	9.7	9.6	9.5	9.5	9.4	9.3	9.2	9.2	9.1
9.5	10.4	10.3	10.3	10.2	10.1	10.0	10.0	9.9	9.8	9.7	9.7	9.6	9.5	9.4	9.4	9.3	9.2	9.1	9.0	9.0
10.0	10.3	10.2	10.1	10.1	10.0	9.9	9.8	9.8	9.7	9.6	9.5	9.5	9.4	9.3	9.2	9.2	9.1	9.0	8.9	8.9

10.5	10.2	10.1	10.0	9.9	9.9	9.8	9.7	9.7	9.6	9.5	9.4	9.4	9.3	9.2	9.1	9.1	9.0	8.9	8.8	8.8
11.0	10.1	10.0	9.9	9.8	9.8	9.7	9.6	9.5	9.5	9.4	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.8	8.7	8.7
11.5	9.9	9.9	9.8	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.2	9.1	9.1	9.0	8.9	8.8	8.8	8.7	8.6	8.6
12.0	9.8	9.8	9.7	9.6	9.5	9.5	9.4	9.3	9.2	9.2	9.1	9.0	9.0	8.9	8.8	8.7	8.7	8.6	8.5	8.5
12.5	9.7	9.6	9.6	9.5	9.4	9.4	9.3	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.7	8.6	8.6	8.5	8.4	8.4

13.0	9.6	9.5	9.5	9.4	9.3	9.3	9.2	9.1	9.0	9.0	8.9	8.8	8.8	8.7	8.6	8.5	8.5	8.4	8.3	8.3
13.5	9.5	9.4	9.4	9.3	9.2	9.1	9.1	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.5	8.5	8.4	8.3	8.2	8.2
14.0	9.4	9.3	9.3	9.2	9.1	9.0	9.0	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.2	8.2	8.1
14.5	9.3	9.2	9.2	9.1	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.1	8.1	8.0
15.0	9.2	9.1	9.1	9.0	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.0	8.0	7.9
15.5	9.1	9.0	9.0	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.8

16.0	9.0	8.9	8.9	8.8	8.7	8.7	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.1	8.1	8.0	7.9	7.9	7.8	7.7
16.5	8.9	8.8	8.8	8.7	8.6	8.6	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.7
17.0	8.8	8.7	8.7	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.6	7.6
17.5	8.7	8.6	8.6	8.5	8.5	8.4	8.3	8.3	8.2	8.1	8.1	8.0	7.9	7.9	7.8	7.7	7.7	7.6	7.6	7.5
18.0	8.6	8.6	8.5	8.4	8.4	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.9	7.8	7.7	7.7	7.6	7.5	7.5	7.4

18.5	8.5	8.5	8.4	8.3	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.7	7.6	7.5	7.5	7.4	7.3
19.0	8.4	8.4	8.3	8.3	8.2	8.1	8.1	8.0	7.9	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.4	7.4	7.3	7.3
19.5	8.4	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.9	7.8	7.7	7.7	7.6	7.6	7.5	7.4	7.4	7.3	7.2	7.2
20.0	8.3	8.2	8.2	8.1	8.0	8.0	7.9	7.8	7.8	7.7	7.7	7.6	7.5	7.5	7.4	7.4	7.3	7.2	7.2	7.1
20.5	8.2	8.1	8.1	8.0	7.9	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.0

21.0	8.1	8.1	8.0	7.9	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.0	7.0
21.5	8.0	8.0	7.9	7.9	7.8	7.7	7.7	7.6	7.6	7.5	7.4	7.4	7.3	7.3	7.2	7.1	7.1	7.0	7.0	6.9
22.0	8.0	7.9	7.8	7.8	7.7	7.7	7.6	7.5	7.5	7.4	7.4	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.8
22.5	7.9	7.8	7.8	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	6.9	6.9	6.8	6.8
23.0	7.8	7.7	7.7	7.6	7.6	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7

23.5	7.7	7.7	7.6	7.6	7.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.0	7.0	6.9	6.9	6.8	6.7	6.7	6.6
24.0	7.7	7.6	7.5	7.5	7.4	7.4	7.3	7.3	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.7	6.7	6.6	6.6
24.5	7.6	7.5	7.5	7.4	7.4	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5
25.0	7.5	7.5	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.4
25.5	7.4	7.4	7.3	7.3	7.2	7.2	7.1	7.1	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.4	6.4

26.0	7.4	7.3	7.3	7.2	7.2	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.5	6.5	6.4	6.4	6.3
26.5	7.3	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3

Temp.	Atmospheric pressure, in millimeters of mercury and (inches of mercury)																			
°C	695 (27.36)	690 (27.17)	685 (26.97)	680 (26.77)	675 (26.57)	670 (26.38)	665 (26.18)	660 (25.98)	655 (25.79)	650 (25.59)	645 (25.39)	640 (25.20)	635 (25.00)	630 (24.80)	625 (24.61)	620 (24.41)	615 (24.21)	610 (24.02)	605 (23.82)	600 (23.62)
27.0	7.2	7.2	7.1	7.1	7.0	7.0	6.9	6.9	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2
27.5	7.2	7.1	7.1	7.0	7.0	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2
28.0	7.1	7.1	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.1	6.1
28.5	7.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.2	6.2	6.1	6.1	6.0
29.0	7.0	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.2	6.2	6.1	6.1	6.0	6.0
29.5	6.9	6.9	6.8	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9
30.0	6.9	6.8	6.8	6.7	6.7	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9

30.5	6.8	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8
31.0	6.7	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8
31.5	6.7	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7
32.0	6.6	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7
32.5	6.6	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6

33.0	6.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6
33.5	6.5	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5
34.0	6.4	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5
34.5	6.4	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4
35.0	6.3	6.3	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4

35.5	6.2	6.2	6.2	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3
36.0	6.2	6.1	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3	5.3
36.5	6.1	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3	5.3	5.2
37.0	6.1	6.1	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3	5.3	5.3	5.2
37.5	6.0	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3	5.3	5.3	5.2	5.2

38.0	6.0	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.3	5.3	5.3	5.2	5.2	5.1
38.5	6.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.4	5.3	5.3	5.2	5.2	5.1	5.1
39.0	5.9	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.4	5.3	5.3	5.2	5.2	5.1	5.1	5.0
39.5	5.9	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.4	5.3	5.3	5.2	5.2	5.1	5.1	5.0	5.0
40.0	5.8	5.8	5.7	5.7	5.6	5.6	5.5	5.5	5.4	5.4	5.4	5.3	5.3	5.2	5.2	5.1	5.1	5.0	5.0	5.0

**Table 2: DO<sub>2</sub> Salinity Correction Factors**

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	0	1000	2000	3000	4000	5000	6000	7000	8000	9000	10000	11000	12000	13000	14000	15000	16000
0.0	1.000	0.996	0.992	0.989	0.985	0.981	0.977	0.973	0.969	0.965	0.961	0.957	0.953	0.950	0.946	0.942	0.938
1.0	1.000	0.996	0.992	0.989	0.985	0.981	0.977	0.973	0.969	0.965	0.962	0.958	0.954	0.950	0.946	0.942	0.938
2.0	1.000	0.996	0.992	0.989	0.985	0.981	0.977	0.973	0.970	0.966	0.962	0.958	0.954	0.950	0.946	0.942	0.938
3.0	1.000	0.996	0.993	0.989	0.985	0.981	0.977	0.974	0.970	0.966	0.962	0.958	0.954	0.951	0.947	0.943	0.939
4.0	1.000	0.996	0.993	0.989	0.985	0.981	0.978	0.974	0.970	0.966	0.962	0.959	0.955	0.951	0.947	0.943	0.939
5.0	1.000	0.996	0.993	0.989	0.985	0.981	0.978	0.974	0.970	0.966	0.963	0.959	0.955	0.951	0.947	0.944	0.940
6.0	1.000	0.996	0.993	0.989	0.985	0.982	0.978	0.974	0.970	0.967	0.963	0.959	0.955	0.952	0.948	0.944	0.940
7.0	1.000	0.996	0.993	0.989	0.985	0.982	0.978	0.974	0.971	0.967	0.963	0.959	0.956	0.952	0.948	0.944	0.941
8.0	1.000	0.996	0.993	0.989	0.986	0.982	0.978	0.975	0.971	0.967	0.963	0.960	0.956	0.952	0.949	0.945	0.941
9.0	1.000	0.996	0.993	0.989	0.986	0.982	0.978	0.975	0.971	0.967	0.964	0.960	0.956	0.953	0.949	0.945	0.941



Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	0	1000	2000	3000	4000	5000	6000	7000	8000	9000	10000	11000	12000	13000	14000	15000	16000
10.0	1.000	0.996	0.993	0.989	0.986	0.982	0.979	0.975	0.971	0.968	0.964	0.960	0.957	0.953	0.949	0.946	0.942
11.0	1.000	0.996	0.993	0.989	0.986	0.982	0.979	0.975	0.971	0.968	0.964	0.961	0.957	0.953	0.950	0.946	0.942
12.0	1.000	0.997	0.993	0.989	0.986	0.982	0.979	0.975	0.972	0.968	0.965	0.961	0.957	0.954	0.950	0.946	0.943
13.0	1.000	0.997	0.993	0.990	0.986	0.983	0.979	0.975	0.972	0.968	0.965	0.961	0.958	0.954	0.950	0.947	0.943
14.0	1.000	0.997	0.993	0.990	0.986	0.983	0.979	0.976	0.972	0.969	0.965	0.961	0.958	0.954	0.951	0.947	0.943

15.0	1.000	0.997	0.993	0.990	0.986	0.983	0.979	0.976	0.972	0.969	0.965	0.962	0.958	0.955	0.951	0.947	0.944
16.0	1.000	0.997	0.993	0.990	0.986	0.983	0.979	0.976	0.972	0.969	0.966	0.962	0.958	0.955	0.951	0.948	0.944
17.0	1.000	0.997	0.993	0.990	0.986	0.983	0.980	0.976	0.973	0.969	0.966	0.962	0.959	0.955	0.952	0.948	0.945
18.0	1.000	0.997	0.993	0.990	0.987	0.983	0.980	0.976	0.973	0.969	0.966	0.963	0.959	0.956	0.952	0.949	0.945
19.0	1.000	0.997	0.993	0.990	0.987	0.983	0.980	0.976	0.973	0.970	0.966	0.963	0.959	0.956	0.952	0.949	0.945

20.0	1.000	0.997	0.993	0.990	0.987	0.983	0.980	0.977	0.973	0.970	0.966	0.963	0.960	0.956	0.953	0.949	0.946
21.0	1.000	0.997	0.993	0.990	0.987	0.984	0.980	0.977	0.973	0.970	0.967	0.963	0.960	0.957	0.953	0.950	0.946
22.0	1.000	0.997	0.993	0.990	0.987	0.984	0.980	0.977	0.974	0.970	0.967	0.964	0.960	0.957	0.953	0.950	0.947
23.0	1.000	0.997	0.994	0.990	0.987	0.984	0.980	0.977	0.974	0.971	0.967	0.964	0.960	0.957	0.954	0.950	0.947
24.0	1.000	0.997	0.994	0.990	0.987	0.984	0.981	0.977	0.974	0.971	0.967	0.964	0.961	0.957	0.954	0.951	0.947

25.0	1.000	0.997	0.994	0.990	0.987	0.984	0.981	0.977	0.974	0.971	0.968	0.964	0.961	0.958	0.954	0.951	0.948
26.0	1.000	0.997	0.994	0.990	0.987	0.984	0.981	0.978	0.974	0.971	0.968	0.965	0.961	0.958	0.955	0.951	0.948
27.0	1.000	0.997	0.994	0.991	0.987	0.984	0.981	0.978	0.975	0.971	0.968	0.965	0.962	0.958	0.955	0.952	0.948
28.0	1.000	0.997	0.994	0.991	0.987	0.984	0.981	0.978	0.975	0.972	0.968	0.965	0.962	0.959	0.955	0.952	0.949
29.0	1.000	0.997	0.994	0.991	0.988	0.984	0.981	0.978	0.975	0.972	0.969	0.965	0.962	0.959	0.956	0.952	0.949
30.0	1.000	0.997	0.994	0.991	0.988	0.985	0.981	0.978	0.975	0.972	0.969	0.966	0.962	0.959	0.956	0.953	0.950
31.0	1.000	0.997	0.994	0.991	0.988	0.985	0.982	0.978	0.975	0.972	0.969	0.966	0.963	0.959	0.956	0.953	0.950
32.0	1.000	0.997	0.994	0.991	0.988	0.985	0.982	0.979	0.975	0.972	0.969	0.966	0.963	0.960	0.957	0.953	0.950
33.0	1.000	0.997	0.994	0.991	0.988	0.985	0.982	0.979	0.976	0.973	0.969	0.966	0.963	0.960	0.957	0.954	0.951
34.0	1.000	0.997	0.994	0.991	0.988	0.985	0.982	0.979	0.976	0.973	0.970	0.967	0.963	0.960	0.957	0.954	0.951

35.0	1.000	0.997	0.994	0.991	0.988	0.985	0.982	0.979	0.976	0.973	0.970	0.967	0.964	0.961	0.957	0.954	0.951
------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------	-------

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	17000	18000	19000	20000	21000	22000	23000	24000	25000	26000	27000	28000	29000	30000	31000	32000	33000
0.0	0.934	0.930	0.926	0.922	0.918	0.914	0.910	0.905	0.901	0.897	0.893	0.889	0.885	0.881	0.877	0.873	0.869
1.0	0.934	0.930	0.926	0.922	0.918	0.914	0.910	0.906	0.902	0.898	0.894	0.890	0.886	0.882	0.878	0.874	0.870
2.0	0.935	0.931	0.927	0.923	0.919	0.915	0.911	0.907	0.903	0.899	0.895	0.891	0.887	0.883	0.879	0.875	0.871
3.0	0.935	0.931	0.927	0.923	0.919	0.915	0.911	0.907	0.903	0.899	0.895	0.891	0.887	0.883	0.879	0.875	0.871
4.0	0.935	0.932	0.928	0.924	0.920	0.916	0.912	0.908	0.904	0.900	0.896	0.892	0.888	0.884	0.880	0.876	0.872

5.0	0.936	0.932	0.928	0.924	0.920	0.917	0.913	0.909	0.905	0.901	0.897	0.893	0.889	0.885	0.881	0.877	0.873
6.0	0.936	0.933	0.929	0.925	0.921	0.917	0.913	0.909	0.905	0.902	0.898	0.894	0.890	0.886	0.882	0.878	0.874
7.0	0.937	0.933	0.929	0.925	0.922	0.918	0.914	0.910	0.906	0.902	0.898	0.894	0.891	0.887	0.883	0.879	0.875
8.0	0.937	0.933	0.930	0.926	0.922	0.918	0.914	0.911	0.907	0.903	0.899	0.895	0.891	0.887	0.884	0.880	0.876

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	17000	18000	19000	20000	21000	22000	23000	24000	25000	26000	27000	28000	29000	30000	31000	32000	33000
9.0	0.938	0.934	0.930	0.926	0.923	0.919	0.915	0.911	0.907	0.904	0.900	0.896	0.892	0.888	0.884	0.880	0.877

10.0	0.938	0.934	0.931	0.927	0.923	0.919	0.916	0.912	0.908	0.904	0.900	0.897	0.893	0.889	0.885	0.881	0.877
11.0	0.939	0.935	0.931	0.927	0.924	0.920	0.916	0.912	0.909	0.905	0.901	0.897	0.894	0.890	0.886	0.882	0.878
12.0	0.939	0.935	0.932	0.928	0.924	0.920	0.917	0.913	0.909	0.906	0.902	0.898	0.894	0.890	0.887	0.883	0.879
13.0	0.939	0.936	0.932	0.928	0.925	0.921	0.917	0.914	0.910	0.906	0.902	0.899	0.895	0.891	0.887	0.884	0.880
14.0	0.940	0.936	0.933	0.929	0.925	0.922	0.918	0.914	0.911	0.907	0.903	0.899	0.896	0.892	0.888	0.884	0.881

15.0	0.940	0.937	0.933	0.929	0.926	0.922	0.918	0.915	0.911	0.907	0.904	0.900	0.896	0.893	0.889	0.885	0.882
16.0	0.941	0.937	0.934	0.930	0.926	0.923	0.919	0.915	0.912	0.908	0.904	0.901	0.897	0.893	0.890	0.886	0.882
17.0	0.941	0.938	0.934	0.930	0.927	0.923	0.920	0.916	0.912	0.909	0.905	0.901	0.898	0.894	0.891	0.887	0.883
18.0	0.942	0.938	0.934	0.931	0.927	0.924	0.920	0.917	0.913	0.909	0.906	0.902	0.899	0.895	0.891	0.888	0.884
19.0	0.942	0.938	0.935	0.931	0.928	0.924	0.921	0.917	0.914	0.910	0.906	0.903	0.899	0.896	0.892	0.888	0.885

20.0	0.942	0.939	0.935	0.932	0.928	0.925	0.921	0.918	0.914	0.911	0.907	0.903	0.900	0.896	0.893	0.889	0.886
21.0	0.943	0.939	0.936	0.932	0.929	0.925	0.922	0.918	0.915	0.911	0.908	0.904	0.901	0.897	0.893	0.890	0.886
22.0	0.943	0.940	0.936	0.933	0.929	0.926	0.922	0.919	0.915	0.912	0.908	0.905	0.901	0.898	0.894	0.891	0.887
23.0	0.944	0.940	0.937	0.933	0.930	0.926	0.923	0.919	0.916	0.912	0.909	0.905	0.902	0.898	0.895	0.891	0.888
24.0	0.944	0.941	0.937	0.934	0.930	0.927	0.923	0.920	0.917	0.913	0.910	0.906	0.903	0.899	0.896	0.892	0.889
25.0	0.944	0.941	0.938	0.934	0.931	0.927	0.924	0.921	0.917	0.914	0.910	0.907	0.903	0.900	0.896	0.893	0.889
26.0	0.945	0.941	0.938	0.935	0.931	0.928	0.925	0.921	0.918	0.914	0.911	0.907	0.904	0.901	0.897	0.894	0.890
27.0	0.945	0.942	0.938	0.935	0.932	0.928	0.925	0.922	0.918	0.915	0.911	0.908	0.905	0.901	0.898	0.894	0.891
28.0	0.946	0.942	0.939	0.936	0.932	0.929	0.926	0.922	0.919	0.915	0.912	0.909	0.905	0.902	0.898	0.895	0.892

29.0	0.946	0.943	0.939	0.936	0.933	0.929	0.926	0.923	0.919	0.916	0.913	0.909	0.906	0.903	0.899	0.896	0.892
30.0	0.946	0.943	0.940	0.936	0.933	0.930	0.927	0.923	0.920	0.917	0.913	0.910	0.907	0.903	0.900	0.896	0.893
31.0	0.947	0.943	0.940	0.937	0.934	0.930	0.927	0.924	0.920	0.917	0.914	0.911	0.907	0.904	0.901	0.897	0.894
32.0	0.947	0.944	0.941	0.937	0.934	0.931	0.928	0.924	0.921	0.918	0.914	0.911	0.908	0.905	0.901	0.898	0.895
33.0	0.947	0.944	0.941	0.938	0.935	0.931	0.928	0.925	0.922	0.918	0.915	0.912	0.908	0.905	0.902	0.899	0.895

34.0	0.948	0.945	0.941	0.938	0.935	0.932	0.929	0.925	0.922	0.919	0.916	0.912	0.909	0.906	0.903	0.899	0.896
35.0	0.948	0.945	0.942	0.939	0.935	0.932	0.929	0.926	0.923	0.919	0.916	0.913	0.910	0.906	0.903	0.900	0.897

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	34000	35000	36000	37000	38000	39000	40000	41000	42000	43000	44000	45000	46000	47000	48000	49000	50000
0.0	0.865	0.861	0.856	0.852	0.848	0.844	0.840	0.836	0.832	0.828	0.823	0.819	0.815	0.811	0.807	0.803	0.799
1.0	0.866	0.862	0.857	0.853	0.849	0.845	0.841	0.837	0.833	0.829	0.825	0.821	0.816	0.812	0.808	0.804	0.800
2.0	0.867	0.862	0.858	0.854	0.850	0.846	0.842	0.838	0.834	0.830	0.826	0.822	0.818	0.814	0.809	0.805	0.801
3.0	0.867	0.863	0.859	0.855	0.851	0.847	0.843	0.839	0.835	0.831	0.827	0.823	0.819	0.815	0.811	0.807	0.803
4.0	0.868	0.864	0.860	0.856	0.852	0.848	0.844	0.840	0.836	0.832	0.828	0.824	0.820	0.816	0.812	0.808	0.804

5.0	0.869	0.865	0.861	0.857	0.853	0.849	0.845	0.841	0.837	0.833	0.829	0.825	0.821	0.817	0.813	0.809	0.805
6.0	0.870	0.866	0.862	0.858	0.854	0.850	0.846	0.842	0.838	0.834	0.830	0.826	0.822	0.818	0.814	0.810	0.806

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	34000	35000	36000	37000	38000	39000	40000	41000	42000	43000	44000	45000	46000	47000	48000	49000	50000
7.0	0.871	0.867	0.863	0.859	0.855	0.851	0.847	0.843	0.839	0.835	0.831	0.828	0.824	0.820	0.816	0.812	0.808
8.0	0.872	0.868	0.864	0.860	0.856	0.852	0.848	0.844	0.840	0.837	0.833	0.829	0.825	0.821	0.817	0.813	0.809
9.0	0.873	0.869	0.865	0.861	0.857	0.853	0.849	0.845	0.842	0.838	0.834	0.830	0.826	0.822	0.818	0.814	0.810

10.0	0.874	0.870	0.866	0.862	0.858	0.854	0.850	0.846	0.843	0.839	0.835	0.831	0.827	0.823	0.819	0.815	0.811
11.0	0.874	0.871	0.867	0.863	0.859	0.855	0.851	0.848	0.844	0.840	0.836	0.832	0.828	0.824	0.820	0.817	0.813
12.0	0.875	0.871	0.868	0.864	0.860	0.856	0.852	0.849	0.845	0.841	0.837	0.833	0.829	0.825	0.822	0.818	0.814
13.0	0.876	0.872	0.869	0.865	0.861	0.857	0.853	0.850	0.846	0.842	0.838	0.834	0.830	0.827	0.823	0.819	0.815
14.0	0.877	0.873	0.869	0.866	0.862	0.858	0.854	0.851	0.847	0.843	0.839	0.835	0.832	0.828	0.824	0.820	0.816

15.0	0.878	0.874	0.870	0.867	0.863	0.859	0.855	0.852	0.848	0.844	0.840	0.836	0.833	0.829	0.825	0.821	0.817
16.0	0.879	0.875	0.871	0.867	0.864	0.860	0.856	0.853	0.849	0.845	0.841	0.838	0.834	0.830	0.826	0.822	0.819
17.0	0.879	0.876	0.872	0.868	0.865	0.861	0.857	0.854	0.850	0.846	0.842	0.839	0.835	0.831	0.827	0.824	0.820
18.0	0.880	0.877	0.873	0.869	0.866	0.862	0.858	0.855	0.851	0.847	0.843	0.840	0.836	0.832	0.829	0.825	0.821
19.0	0.881	0.877	0.874	0.870	0.867	0.863	0.859	0.855	0.852	0.848	0.844	0.841	0.837	0.833	0.830	0.826	0.822
20.0	0.882	0.878	0.875	0.871	0.867	0.864	0.860	0.856	0.853	0.849	0.845	0.842	0.838	0.834	0.831	0.827	0.823
21.0	0.883	0.879	0.876	0.872	0.868	0.865	0.861	0.857	0.854	0.850	0.846	0.843	0.839	0.836	0.832	0.828	0.825
22.0	0.884	0.880	0.876	0.873	0.869	0.866	0.862	0.858	0.855	0.851	0.848	0.844	0.840	0.837	0.833	0.829	0.826

23.0	0.884	0.881	0.877	0.874	0.870	0.866	0.863	0.859	0.856	0.852	0.849	0.845	0.841	0.838	0.834	0.830	0.827
24.0	0.885	0.882	0.878	0.874	0.871	0.867	0.864	0.860	0.857	0.853	0.850	0.846	0.842	0.839	0.835	0.832	0.828
25.0	0.886	0.882	0.879	0.875	0.872	0.868	0.865	0.861	0.858	0.854	0.851	0.847	0.843	0.840	0.836	0.833	0.829
26.0	0.887	0.883	0.880	0.876	0.873	0.869	0.866	0.862	0.859	0.855	0.852	0.848	0.844	0.841	0.837	0.834	0.830
27.0	0.887	0.884	0.880	0.877	0.874	0.870	0.867	0.863	0.860	0.856	0.853	0.849	0.845	0.842	0.838	0.835	0.831

28.0	0.888	0.885	0.881	0.878	0.874	0.871	0.867	0.864	0.860	0.857	0.853	0.850	0.846	0.843	0.839	0.836	0.832
29.0	0.889	0.886	0.882	0.879	0.875	0.872	0.868	0.865	0.861	0.858	0.854	0.851	0.848	0.844	0.841	0.837	0.834
30.0	0.890	0.886	0.883	0.879	0.876	0.873	0.869	0.866	0.862	0.859	0.855	0.852	0.849	0.845	0.842	0.838	0.835
31.0	0.890	0.887	0.884	0.880	0.877	0.873	0.870	0.867	0.863	0.860	0.856	0.853	0.850	0.846	0.843	0.839	0.836
32.0	0.891	0.888	0.884	0.881	0.878	0.874	0.871	0.868	0.864	0.861	0.857	0.854	0.851	0.847	0.844	0.840	0.837

33.0	0.892	0.889	0.885	0.882	0.879	0.875	0.872	0.868	0.865	0.862	0.858	0.855	0.851	0.848	0.845	0.841	0.838
34.0	0.893	0.889	0.886	0.883	0.879	0.876	0.873	0.869	0.866	0.863	0.859	0.856	0.852	0.849	0.846	0.842	0.839
35.0	0.893	0.890	0.887	0.883	0.880	0.877	0.874	0.870	0.867	0.863	0.860	0.857	0.853	0.850	0.847	0.843	0.840

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	51000	52000	53000	54000	55000	56000	57000	58000	59000	60000	61000	62000	63000	64000	65000	66000	67000
0.0	0.795	0.790	0.786	0.782	0.778	0.774	0.770	0.766	0.761	0.757	0.753	0.749	0.745	0.741	0.737	0.732	0.728
1.0	0.796	0.792	0.788	0.783	0.779	0.775	0.771	0.767	0.763	0.759	0.755	0.751	0.746	0.742	0.738	0.734	0.730
2.0	0.797	0.793	0.789	0.785	0.781	0.777	0.773	0.768	0.764	0.760	0.756	0.752	0.748	0.744	0.740	0.736	0.732
3.0	0.798	0.794	0.790	0.786	0.782	0.778	0.774	0.770	0.766	0.762	0.758	0.754	0.750	0.746	0.741	0.737	0.733
4.0	0.800	0.796	0.792	0.788	0.784	0.780	0.775	0.771	0.767	0.763	0.759	0.755	0.751	0.747	0.743	0.739	0.735

Temp.	Conductivity, in microsiemens per centimeter at 25 degrees Celsius																
°C	51000	52000	53000	54000	55000	56000	57000	58000	59000	60000	61000	62000	63000	64000	65000	66000	67000
5.0	0.801	0.797	0.793	0.789	0.785	0.781	0.777	0.773	0.769	0.765	0.761	0.757	0.753	0.749	0.745	0.741	0.737
6.0	0.802	0.798	0.794	0.790	0.786	0.782	0.778	0.774	0.770	0.766	0.762	0.758	0.754	0.750	0.746	0.742	0.738
7.0	0.804	0.800	0.796	0.792	0.788	0.784	0.780	0.776	0.772	0.768	0.764	0.760	0.756	0.752	0.748	0.744	0.740
8.0	0.805	0.801	0.797	0.793	0.789	0.785	0.781	0.777	0.773	0.769	0.765	0.761	0.757	0.753	0.749	0.745	0.742
9.0	0.806	0.802	0.798	0.794	0.790	0.787	0.783	0.779	0.775	0.771	0.767	0.763	0.759	0.755	0.751	0.747	0.743

10.0	0.807	0.804	0.800	0.796	0.792	0.788	0.784	0.780	0.776	0.772	0.768	0.764	0.760	0.757	0.753	0.749	0.745
11.0	0.809	0.805	0.801	0.797	0.793	0.789	0.785	0.781	0.778	0.774	0.770	0.766	0.762	0.758	0.754	0.750	0.746
12.0	0.810	0.806	0.802	0.798	0.794	0.791	0.787	0.783	0.779	0.775	0.771	0.767	0.763	0.760	0.756	0.752	0.748
13.0	0.811	0.807	0.804	0.800	0.796	0.792	0.788	0.784	0.780	0.777	0.773	0.769	0.765	0.761	0.757	0.753	0.750
14.0	0.812	0.809	0.805	0.801	0.797	0.793	0.789	0.786	0.782	0.778	0.774	0.770	0.766	0.763	0.759	0.755	0.751
15.0	0.814	0.810	0.806	0.802	0.798	0.795	0.791	0.787	0.783	0.779	0.776	0.772	0.768	0.764	0.760	0.756	0.753
16.0	0.815	0.811	0.807	0.804	0.800	0.796	0.792	0.788	0.785	0.781	0.777	0.773	0.769	0.766	0.762	0.758	0.754

17.0	0.816	0.812	0.809	0.805	0.801	0.797	0.794	0.790	0.786	0.782	0.778	0.775	0.771	0.767	0.763	0.760	0.756
18.0	0.817	0.814	0.810	0.806	0.802	0.799	0.795	0.791	0.787	0.784	0.780	0.776	0.772	0.769	0.765	0.761	0.757
19.0	0.819	0.815	0.811	0.807	0.804	0.800	0.796	0.792	0.789	0.785	0.781	0.777	0.774	0.770	0.766	0.763	0.759
20.0	0.820	0.816	0.812	0.809	0.805	0.801	0.797	0.794	0.790	0.786	0.783	0.779	0.775	0.771	0.768	0.764	0.760
21.0	0.821	0.817	0.814	0.810	0.806	0.802	0.799	0.795	0.791	0.788	0.784	0.780	0.777	0.773	0.769	0.766	0.762

22.0	0.822	0.818	0.815	0.811	0.807	0.804	0.800	0.796	0.793	0.789	0.785	0.782	0.778	0.774	0.771	0.767	0.763
23.0	0.823	0.820	0.816	0.812	0.809	0.805	0.801	0.798	0.794	0.790	0.787	0.783	0.779	0.776	0.772	0.768	0.765
24.0	0.824	0.821	0.817	0.814	0.810	0.806	0.803	0.799	0.795	0.792	0.788	0.785	0.781	0.777	0.774	0.770	0.766
25.0	0.826	0.822	0.818	0.815	0.811	0.808	0.804	0.800	0.797	0.793	0.789	0.786	0.782	0.779	0.775	0.771	0.768
26.0	0.827	0.823	0.820	0.816	0.812	0.809	0.805	0.802	0.798	0.794	0.791	0.787	0.784	0.780	0.776	0.773	0.769

27.0	0.828	0.824	0.821	0.817	0.814	0.810	0.806	0.803	0.799	0.796	0.792	0.789	0.785	0.781	0.778	0.774	0.771
28.0	0.829	0.825	0.822	0.818	0.815	0.811	0.808	0.804	0.801	0.797	0.794	0.790	0.786	0.783	0.779	0.776	0.772
29.0	0.830	0.827	0.823	0.820	0.816	0.812	0.809	0.805	0.802	0.798	0.795	0.791	0.788	0.784	0.781	0.777	0.774
30.0	0.831	0.828	0.824	0.821	0.817	0.814	0.810	0.807	0.803	0.800	0.796	0.793	0.789	0.786	0.782	0.779	0.775
31.0	0.832	0.829	0.825	0.822	0.818	0.815	0.811	0.808	0.804	0.801	0.797	0.794	0.790	0.787	0.783	0.780	0.776

32.0	0.833	0.830	0.826	0.823	0.820	0.816	0.813	0.809	0.806	0.802	0.799	0.795	0.792	0.788	0.785	0.781	0.778
33.0	0.834	0.831	0.828	0.824	0.821	0.817	0.814	0.810	0.807	0.803	0.800	0.797	0.793	0.790	0.786	0.783	0.779
34.0	0.836	0.832	0.829	0.825	0.822	0.818	0.815	0.812	0.808	0.805	0.801	0.798	0.794	0.791	0.788	0.784	0.781
35.0	0.837	0.833	0.830	0.826	0.823	0.820	0.816	0.813	0.809	0.806	0.803	0.799	0.796	0.792	0.789	0.785	0.782

## Technical Support

For assistance with any PASCO product, contact PASCO at:

Address: PASCO scientific  
10101 Foothills Blvd.  
Roseville, CA 95747-7100

Phone: 916-786-3800 (worldwide)  
800-772-8700 (U.S.)

Fax: (916) 786-3292

Web: [www.pasco.com](http://www.pasco.com)

Email: [support@pasco.com](mailto:support@pasco.com)

### Limited Warranty

For a description of the product warranty, see the PASCO catalog.

### Copyright

The PASCO scientific 012-09384D *Water Quality MultiMeasure Sensor Instruction Manual* is copyrighted with all rights reserved. Permission is granted to non-profit educational institutions for reproduction of any part of this manual, providing the reproductions are used only in their laboratories and classrooms, and are not sold for profit. Reproduction under any other circumstances, without the written consent of PASCO scientific, is prohibited.

### Trademarks

PASCO, PASCO scientific, DataStudio, MultiMeasure Sensors, PASPORT, and ScienceWorkshop are trademarks or registered trademarks of PASCO scientific, in the United States and/or in other countries. All other brands, products, or service names are or may be trademarks or service marks of, and are used to identify, products or services of, their respective owners. For more information visit [www.pasco.com/legal](http://www.pasco.com/legal). Teflon is a registered trademark of DuPont.